




12/01/2012

Histogram of Samples

Measurement mode : Period Ch2

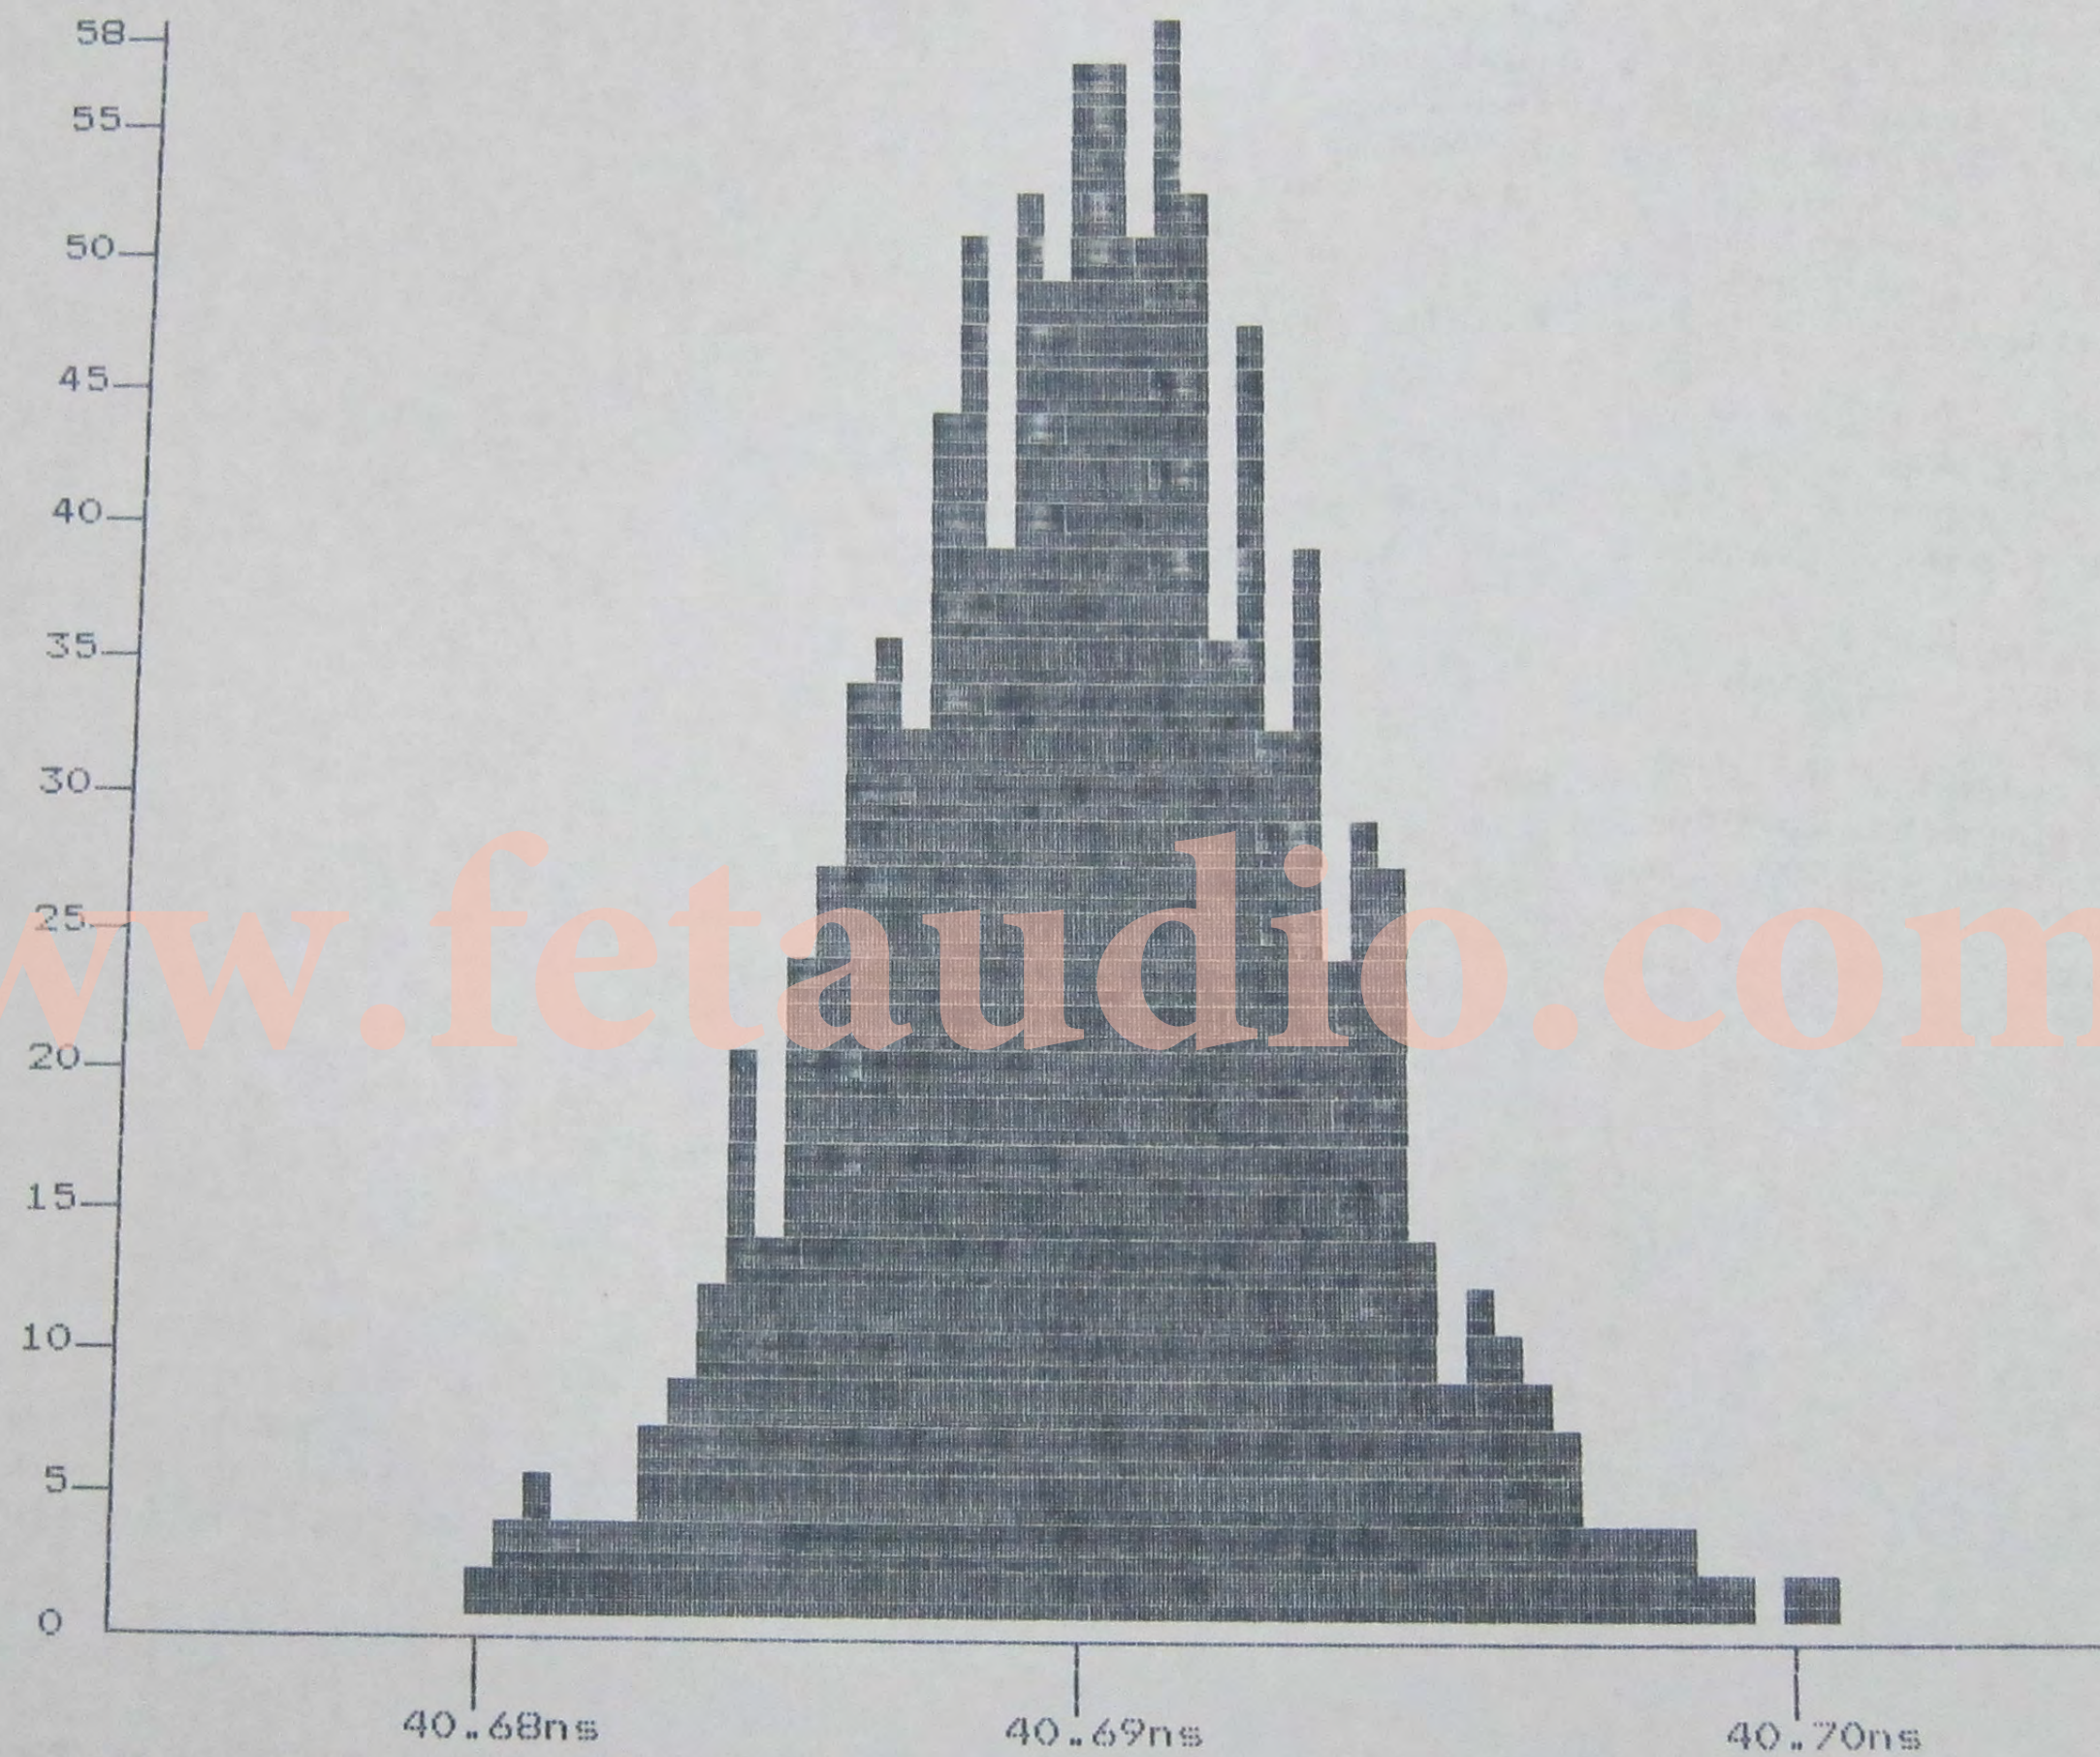

Test Results

Samples : 1000
Sets : 1
Measured : 40,689.409ps
Maximum : 40705ps
Minimum : 40676ps
Range : 14.34ps
Jitter : 4.600ps

12/01/2012

Wave Technologies DTS-2070 Ver. 3.5
Part #: Serial #:0

Current Test Configuration

Measurement mode : Period Ch2
Samples : 1000
Sets : 1
Triggering : Automatic
Gating with ARM2 : Disabled
User trip levels : Disabled
Trip levels : 50%-50%
Event sequence : Arm On Stop
Start arming cnt : 1
Stop arming cnt : 2
Filtering : Disabled

Trip Voltages

Start event : -0.0148
Stop event : -0.0148
CH2 peak voltages : +1.0195 -1.0491

Test Results

Samples : 1000
Sets : 1
Measured : 40,689.409ps
Maximum : 40705ps
Minimum : 40676ps
Range : 14.34ps
Jitter : 4.600ps

12/01/2012